




HAEMATOLOGY ANALYSERS

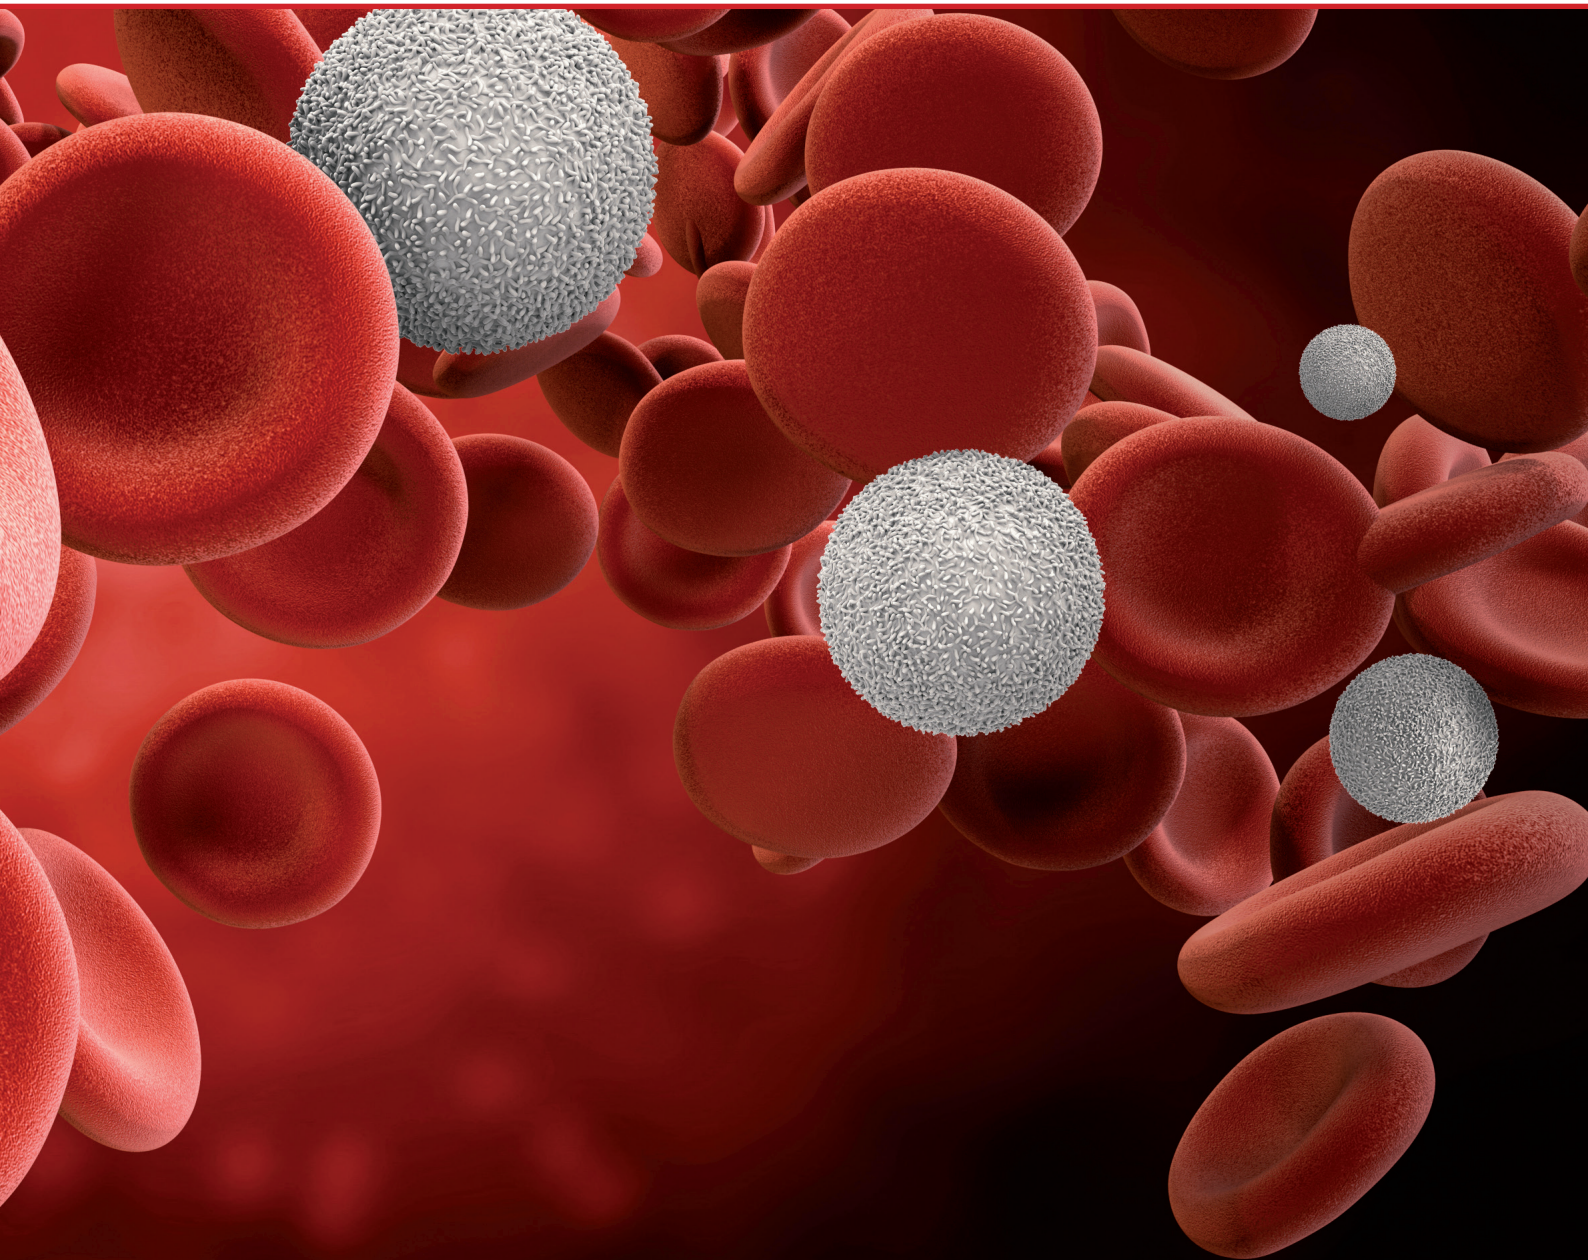

DLB5

5-diff Haematology Analyser

-
- 1 Analyser - 2 functions: switch between 3-diff and 5-diff
 - 18 parameters + 3 histograms (3-diff):
WBC, RBC, THR, Hb, Hct, Lym%, Lym#, Mon%, Mon#, Gra%, Gra#, MCV, MCH, MCHC, RDW, MPV, Pct, PDW
 - 21 parameters + 4 histograms (5-diff):
WBC, RBC, THR, Hb, Hct, Lym%, Lym#, Mon%, Mon#, Neu%, Neu#, Eo%, Eo#, Ba%, MCV, MCH, MCHC, RDW, MPV, Pct, PDW
-


DLB3

3-diff Haematology Analyser

-
- 18 parameters + 3 histograms:
WBC, RBC, THR, Hb, Hct, Lym%, Lym#, Mon%, Mon#, Gra%, Gra#, MCV, MCH, MCHC, RDW, MPV, Pct, PDW
-

General Features for DLB5 and DLB3

-
- Results in 50 seconds (3-diff) or 80 seconds (5-diff)
 - For venous and capillary blood
 - Only 10 – 30 µL blood volume
 - No warm-up, temperature independent
 - Colour display
 - Printer: DLB5 internal, DLB3 external (not included)
 - Connection to external computer, keyboard and barcode reader
 - 5-diff: 4 reagents plus Rinse, 3-diff: 3 reagents plus Rinse
 - Blood Clot Micro Filter
 - Unique preservation solution » no frequent rinsing
 - Electromagnetic valves » less service needed
 - Cleaning every 3 months only
 - Service once a year
 - Languages: German, English, French (Spanish on request)
 - Veterinary instrument: 6 species by default, 2 species freely selectable
-



Order Information

Human

Instruments	Description	Warranty	REF
DLB3	3-diff	5 years	H19100
DLB5	5-diff	5 years	H19110

Reagents	Description	Content	REF
Diadiff	for DLB5 and DLB3	1,2 L (1000 cycles)	H19150
Dialuent	for DLB5 and DLB3	20 L (1000 cycles)	H19120
Diatergent	for DLB5 and DLB3	5 L (1000 cycles)	H19130
Dialys-E0	for DLB5	5 L (1000 cycles)	H19160
Rinse Concentrate	for DLB5 and DLB3	0,25 L	H19140C
DLB3 Pack 125H	3-diff	125 cycles	H19261
DLB5 Pack 125H	5-diff	125 cycles	H19262

Stability from date of production: 3 years | Open stability: 4 months


Veterinary

Instruments	Description	Warranty	REF
DLB3 VET	3-diff	5 years	H19800
DLB5 VET	5-diff	5 years	H19810

Reagents	Description	Content	REF
Diadiff VET	for DLB5 VET	1,2 L (1000 cycles)	H19240
Dialuent VET	for DLB5 VET and DLB3 VET	20 L (1000 cycles)	H19220
Diatergent VET	for DLB5 VET and DLB3 VET	5 L (1000 cycles)	H19230
Dialys-E0 VET	for DLB5 VET	5 L (1000 cycles)	H19260
Rinse Concentrate	for DLB5 VET and DLB3 VET	0,25 L	H19140C
DLB3 Pack 125V	3-diff	125 cycles	H19271
DLB5 Pack 125V	5-diff	125 cycles	H19272

Stability from date of production: 3 years | Open stability: 4 months



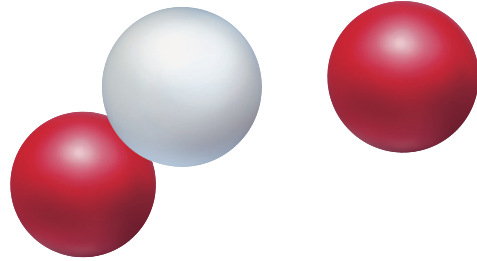

DIALAB®

Austria

DIALAB® GmbH

IZ NOE-Sued

Hondastrasse, Objekt M55

A-2351 Wiener Neudorf

Phone: +43-2236-66 09 10-0

Fax: +43-2236-66 09 10-30

E-mail: office@dialab.at

www.dialab.at